



# DM-6D

## HEMATOLOGY CONTROL

Reference Values provided by DYMIND


**CONTROL**
 2022-11-13

 2023-02-10


Instruments	Parameter	Unit	LOT	6D1222L	LOT	6D1222N	LOT	6D1222H
DYMIND  DH-600 DH-602 DH-605 DH-610 DH-612 DH-615  (Technical File Version A1.0 or higher)	<b>WBC</b>	×10 <sup>9</sup> /L	<b>4.19</b>	±1.20	<b>7.64</b>	±1.80	<b>21.99</b>	±3.00
	Neu#	×10 <sup>9</sup> /L	2.89	±0.40	4.64	±0.80	15.83	±2.00
	Lym#	×10 <sup>9</sup> /L	0.64	±0.40	2.05	±0.70	4.31	±1.80
	Mon#	×10 <sup>9</sup> /L	0.42	±0.40	0.56	±0.50	0.91	±0.80
	Eos#	×10 <sup>9</sup> /L	0.25	±0.40	0.39	±0.70	0.94	±1.60
	Bas#	×10 <sup>9</sup> /L	3.36	±0.40	5.53	±0.70	16.48	±1.60
	IG#	×10 <sup>9</sup> /L	0.54	±0.50	0.91	±1.00	2.86	±2.50
	Neu%	%	68.8	±12.0	60.6	±12.0	71.9	±12.0
	Lym%	%	15.1	±10.0	26.9	±10.0	19.6	±10.0
	Mon%	%	10.0	±8.0	7.4	±8.0	4.2	±8.0
	Eos%	%	6.0	±10.0	5.1	±10.0	4.3	±10.0
	Bas%	%	80.2	±10.0	72.4	±10.0	74.9	±10.0
	IG%	%	12.9	±10.0	12.0	±10.0	13.0	±10.0
	<b>RBC</b>	×10 <sup>12</sup> /L	<b>2.53</b>	±0.20	<b>4.69</b>	±0.30	<b>5.68</b>	±0.50
	<b>HGB</b>	g/L	<b>67</b>	±4	<b>141</b>	±6	<b>181</b>	±8
	HCT	%	19.4	±2.0	41.6	±2.5	52.9	±3.0
	<b>MCV</b>	fL	<b>76.8</b>	±5.0	<b>88.8</b>	±5.0	<b>93.3</b>	±5.0
	MCH	pg	26.4	±2.5	30.0	±2.5	31.9	±2.5
	MCHC	g/L	343	±30	338	±30	341	±30
	RDW-CV	%	16.0	±5.0	14.6	±5.0	14.3	±6.0
RDW-SD	fL	44.6	±10.0	47.2	±10.0	48.3	±12.0	
<b>PLT</b>	×10 <sup>9</sup> /L	<b>74</b>	±20	<b>262</b>	±45	<b>555</b>	±65	
MPV	fL	8.2	±3.0	8.3	±3.0	8.5	±3.0	
PDW	fL	8.3	±5.0	8.9	±5.0	9.6	±5.0	
PCT	%	0.061	±0.050	0.218	±0.100	0.472	±0.200	
P-LCR	%	15.3	±20.0	14.3	±20.0	16.0	±20.0	
P-LCC	×10 <sup>9</sup> /L	11	±10	38	±30	89	±50	
IPF	%	2.3	±2.3	2.6	±2.6	2.5	±2.5	

**【NOTE】**


1. The controls should be stored in refrigerator (2°C~8°C). After opening, it will keep stable for 14 days when it is stored airtight at 2°C~8°C.
2. Before mixing and running the control after take it out from the refrigerator, please keep it at least 15 minutes until reaching room temperature(15°C~30°C).
3. Controls must be well mixed before using. Please mix gently, to avoid cells rupture and/or generating bubbles.
4. After using, put the controls back into the refrigerator to prevent contamination and evaporation.

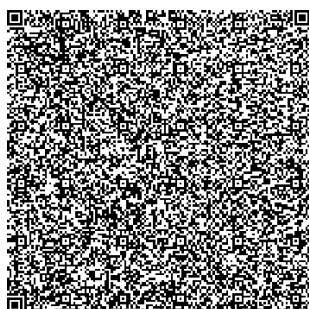

6D1222L

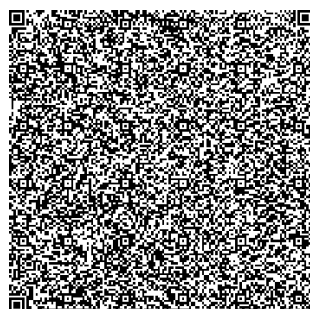

6D1222N

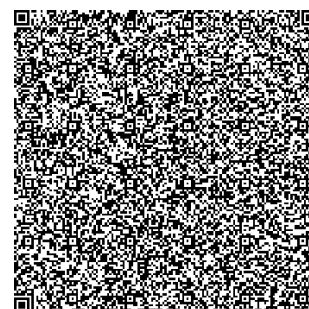

6D1222H