

DM-6D

HEMATOLOGY CONTROL

Reference Values provided by DYMIND

CONTROL


📅 2023-01-11

📅 2023-04-10


Instruments	Parameter	Unit	LOT	6D0223L	LOT	6D0223N	LOT	6D0223H
DYMIND DH-600 DH-602 DH-605 DH-610 DH-612 DH-615 (Technical File Version A1.0 or higher)	WBC	×10 ⁹ /L	4.02	±1.20	7.66	±1.80	21.52	±3.00
	Neu#	×10 ⁹ /L	2.91	±0.40	4.86	±0.80	15.69	±2.00
	Lym#	×10 ⁹ /L	0.55	±0.40	1.97	±0.70	4.21	±1.80
	Mon#	×10 ⁹ /L	0.39	±0.40	0.57	±0.50	0.94	±0.80
	Eos#	×10 ⁹ /L	0.17	±0.40	0.26	±0.70	0.69	±1.60
	Bas#	×10 ⁹ /L	3.24	±0.40	5.57	±0.70	15.94	±1.60
	IG#	×10 ⁹ /L	0.53	±0.50	0.92	±1.00	2.88	±2.50
	Neu%	%	72.0	±12.0	63.1	±12.0	72.6	±12.0
	Lym%	%	13.8	±10.0	25.9	±10.0	19.8	±10.0
	Mon%	%	9.8	±8.0	7.5	±8.0	4.4	±8.0
	Eos%	%	4.5	±10.0	3.5	±10.0	3.2	±10.0
	Bas%	%	81.4	±10.0	73.5	±10.0	74.8	±10.0
	IG%	%	13.3	±10.0	12.1	±10.0	13.5	±10.0
	RBC	×10 ¹² /L	2.37	±0.20	4.47	±0.30	5.22	±0.50
	HGB	g/L	61	±4	134	±6	169	±8
	HCT	%	18.3	±2.0	40.6	±2.5	50.4	±3.0
	MCV	fL	77.5	±5.0	90.8	±5.0	96.5	±5.0
	MCH	pg	25.8	±2.5	29.9	±2.5	32.3	±2.5
	MCHC	g/L	333	±30	329	±30	335	±30
	RDW-CV	%	17.0	±5.0	14.6	±5.0	14.5	±6.0
	RDW-SD	fL	46.4	±10.0	47.2	±10.0	49.7	±12.0
	PLT	×10 ⁹ /L	61	±20	276	±45	553	±65
	MPV	fL	7.9	±3.0	7.5	±3.0	7.3	±3.0
	PDW	fL	10.8	±5.0	8.6	±5.0	8.6	±5.0
	PCT	%	0.048	±0.050	0.206	±0.100	0.405	±0.200
	P-LCR	%	14.8	±20.0	11.8	±20.0	10.7	±20.0
	P-LCC	×10 ⁹ /L	9	±10	32	±30	59	±50
IPF	%	2.3	±2.3	2.2	±2.6	1.6	±2.5	

【NOTE】


1. The controls should be stored in refrigerator (2°C~8°C). After opening, it will keep stable for 14 days when it is stored airtight at 2°C~8°C.
2. Before mixing and running the control after take it out from the refrigerator, please keep it at least 15 minutes until reaching room temperature(15°C~30°C).
3. Controls must be well mixed before using. Please mix gently, to avoid cells rupture and/or generating bubbles.
4. After using, put the controls back into the refrigerator to prevent contamination and evaporation.

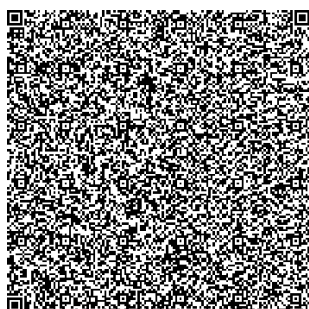

6D0223L

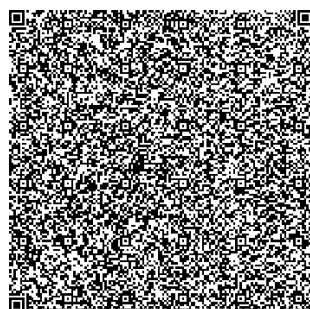

6D0223N

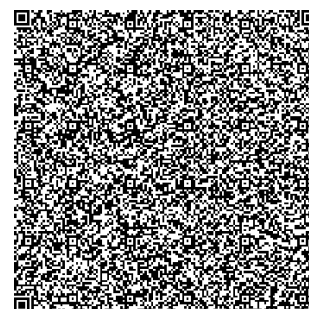

6D0223H