

	文件类型	技术文件	文件版本	V3.2.0	
	项目代号	/	页 码	第 0 页 共 1 页	
	文件编号	GL DM-56-18-en			
文件名称： <p style="text-align: center;">CONTROL DM-6D 6D0423 2023-06-10</p> 适用范围：1116 项目					
编制：		审核：		批准：	
日期：		日期：		日期：	
修 订 记 录					
版本	TCN/ECR/PCN 编号	修订内容概要	修改人	批准人	批准日期
V3.2.0	/	新建	刘嘉	郑剑通	2023.03.27
发至：	<input type="checkbox"/> 总经办 <input type="checkbox"/> 质量部 <input type="checkbox"/> 财务部 <input checked="" type="checkbox"/> 营销部 <input checked="" type="checkbox"/> 客服 <input type="checkbox"/> 计划 <input type="checkbox"/> 采购 <input checked="" type="checkbox"/> 工程 <input type="checkbox"/> 仓库 <input checked="" type="checkbox"/> 设备研发 <input checked="" type="checkbox"/> 试剂研发 <input type="checkbox"/> 物料质量 <input type="checkbox"/> 设备生产 <input type="checkbox"/> 试剂生产 <input checked="" type="checkbox"/> 试剂质检 <input checked="" type="checkbox"/> 设备质检				
由试剂研发					

DM-6D

HEMATOLOGY CONTROL

Reference Values provided by DYMIND


CONTROL
 2023-03-13

 2023-06-10


Instruments	Parameter	Unit	LOT	6D0423L	LOT	6D0423N	LOT	6D0423H
DYMIND DH-600 DH-602 DH-605 DH-610 DH-612 DH-615 (Technical File Version A1.6 or higher)	WBC	×10 ⁹ /L	4.56	±1.20	7.83	±1.80	22.51	±3.00
	Neu#	×10 ⁹ /L	3.27	±0.40	4.92	±0.80	16.15	±2.00
	Lym#	×10 ⁹ /L	0.72	±0.40	2.16	±0.70	4.72	±1.80
	Mon#	×10 ⁹ /L	0.36	±0.40	0.46	±0.50	0.88	±0.80
	Eos#	×10 ⁹ /L	0.20	±0.40	0.29	±0.70	0.77	±1.60
	Bas#	×10 ⁹ /L	3.64	±0.40	5.71	±0.70	16.76	±1.60
	IG#	×10 ⁹ /L	0.61	±0.50	0.97	±1.00	2.89	±2.50
	Neu%	%	71.8	±12.0	62.8	±12.0	71.7	±12.0
	Lym%	%	15.8	±10.0	27.6	±10.0	21.0	±10.0
	Mon%	%	8.0	±8.0	5.9	±8.0	3.9	±8.0
	Eos%	%	4.4	±10.0	3.8	±10.0	3.4	±10.0
	Bas%	%	79.9	±10.0	72.9	±10.0	74.5	±10.0
	IG%	%	13.4	±10.0	12.4	±10.0	12.8	±10.0
	RBC	×10 ¹² /L	2.34	±0.20	4.62	±0.30	5.48	±0.50
	HGB	g/L	62	±4	135	±6	175	±8
	HCT	%	18.4	±2.0	40.9	±2.5	52.9	±3.0
	MCV	fL	78.8	±5.0	88.5	±5.0	96.5	±5.0
	MCH	pg	26.4	±2.5	29.2	±2.5	31.9	±2.5
	MCHC	g/L	340	±30	335	±30	336	±30
	RDW-CV	%	16.6	±5.0	15.0	±5.0	14.4	±6.0
	RDW-SD	fL	46.0	±10.0	46.8	±10.0	48.8	±12.0
	PLT	×10 ⁹ /L	66	±20	292	±45	535	±65
	MPV	fL	7.1	±3.0	7.0	±3.0	7.2	±3.0
	PDW	fL	8.3	±5.0	8.4	±5.0	8.9	±5.0
	PCT	%	0.047	±0.050	0.204	±0.100	0.386	±0.200
	P-LCR	%	9.7	±20.0	8.6	±20.0	9.4	±20.0
	P-LCC	×10 ⁹ /L	6	±10	25	±30	51	±50
IPF	%	1.9	±1.9	1.8	±1.8	1.7	±1.7	

【NOTE】


1. The controls should be stored in refrigerator (2°C~8°C). After opening, it will keep stable for 14 days when it is stored airtight at 2°C~8°C.
2. Before mixing and running the control after take it out from the refrigerator, please keep it at least 15 minutes until reaching room temperature(15°C~30°C).
3. Controls must be well mixed before using. Please mix gently, to avoid cells rupture and/or generating bubbles.
4. After using, put the controls back into the refrigerator to prevent contamination and evaporation.

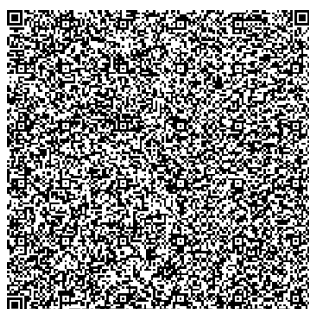

6D0423L

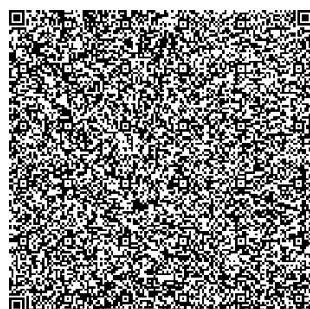

6D0423N

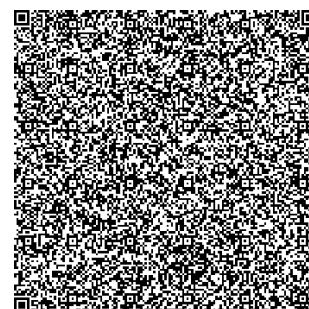

6D0423H