

	文件类型	技术文件	文件版本	V3.3.0	
	项目代号	/	页 码	第 0 页 共 1 页	
	文件编号	GL DM-56-18-en			
文件名称： <p style="text-align: center;">CONTROL DM-6D 6D0623 2023-08-10</p> 适用范围：1116 项目					
编制：石丽岐 日期：2023.05.31		审核：郑剑通 日期：2023.05.31		批准：郑剑通 日期：2023.05.31	
修 订 记 录					
版本	TCN/ECR/PCN 编号	修订内容概要	修改人	批准人	批准日期
V3.3.0	/	新建	石丽岐	郑剑通	2023.05.31
发至：	<input type="checkbox"/> 总经办 <input type="checkbox"/> 质量部 <input type="checkbox"/> 财务部 <input checked="" type="checkbox"/> 营销部 <input checked="" type="checkbox"/> 客服 <input type="checkbox"/> 计划 <input type="checkbox"/> 采购 <input checked="" type="checkbox"/> 工程 <input type="checkbox"/> 仓库 <input checked="" type="checkbox"/> 设备研发 <input checked="" type="checkbox"/> 试剂研发 <input type="checkbox"/> 物料质量 <input type="checkbox"/> 设备生产 <input type="checkbox"/> 试剂生产 <input checked="" type="checkbox"/> 试剂质检 <input checked="" type="checkbox"/> 设备质检				
由试剂研发					

DM-6D

HEMATOLOGY CONTROL

Reference Values provided by DYMIND


CONTROL
 2023-05-13

 2023-08-10


Instruments	Parameter	Unit	LOT	6D0623L	LOT	6D0623N	LOT	6D0623H
DYMIND	WBC	×10 ⁹ /L	4.02	±1.20	7.84	±1.80	21.89	±3.00
	Neu#	×10 ⁹ /L	2.93	±0.40	4.95	±0.80	15.53	±2.00
DH-600	Lym#	×10 ⁹ /L	0.56	±0.40	2.06	±0.70	4.46	±1.80
DH-602	Mon#	×10 ⁹ /L	0.34	±0.40	0.53	±0.50	0.88	±0.80
DH-605	Eos#	×10 ⁹ /L	0.19	±0.40	0.30	±0.70	1.01	±1.60
DH-610	Bas#	×10 ⁹ /L	3.26	±0.40	5.79	±0.70	16.21	±1.60
DH-612	IG#	×10 ⁹ /L	0.53	±0.50	0.95	±1.00	2.65	±2.50
DH-615	Neu%	%	72.8	±12.0	63.2	±12.0	71.0	±12.0
(Technical File Version A2.0 or higher)	Lym%	%	14.0	±10.0	26.3	±10.0	20.4	±10.0
	Mon%	%	8.4	±8.0	6.7	±8.0	4.0	±8.0
	Eos%	%	4.8	±10.0	3.8	±10.0	4.6	±10.0
	Bas%	%	81.0	±10.0	73.8	±10.0	74.1	±10.0
	IG%	%	13.3	±10.0	12.2	±10.0	12.1	±10.0
	RBC	×10 ¹² /L	2.30	±0.20	4.50	±0.30	5.55	±0.50
	HGB	g/L	61	±4	134	±6	179	±8
	HCT	%	17.4	±2.0	39.0	±2.5	51.9	±3.0
	MCV	fL	75.8	±5.0	86.8	±5.0	93.5	±5.0
	MCH	pg	26.6	±2.5	29.7	±2.5	32.2	±2.5
	MCHC	g/L	351	±30	342	±30	344	±30
	RDW-CV	%	17.1	±5.0	15.3	±5.0	14.6	±6.0
	RDW-SD	fL	47.8	±10.0	49.1	±10.0	50.5	±12.0
	PLT	×10 ⁹ /L	71	±20	300	±45	558	±65
	MPV	fL	7.8	±3.0	7.3	±3.0	7.3	±3.0
	PDW	fL	9.7	±5.0	8.5	±5.0	8.8	±5.0
	PCT	%	0.056	±0.050	0.219	±0.100	0.407	±0.200
	P-LCR	%	14.0	±20.0	10.7	±20.0	10.3	±20.0
	P-LCC	×10 ⁹ /L	10	±10	32	±30	58	±50
	IPF	%	2.1	±2.1	2.3	±2.3	2.0	±2.0

【NOTE】


1. The controls should be stored in refrigerator (2°C~8°C). After opening, it will keep stable for 14 days when it is stored airtight at 2°C~8°C.
2. Before mixing and running the control after take it out from the refrigerator, please keep it at least 15 minutes until reaching room temperature(15°C~30°C).
3. Controls must be well mixed before using. Please mix gently, to avoid cells rupture and/or generating bubbles.
4. After using, put the controls back into the refrigerator to prevent contamination and evaporation.

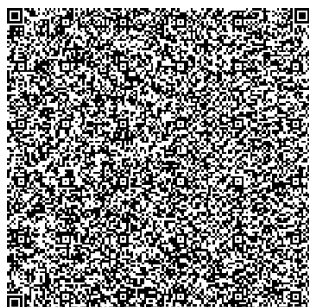

6D0623L

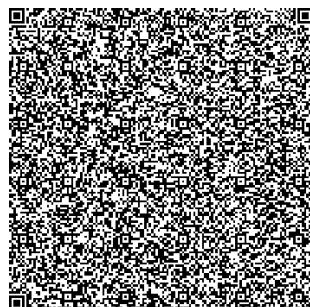

6D0623N

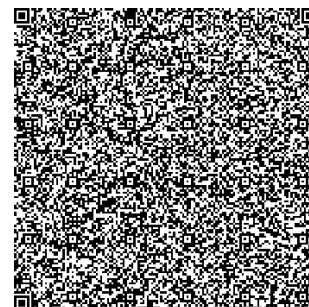

6D0623H