

	文件类型	技术文件	文件版本	V3.5.0	
	项目代号	/	页 码	第 0 页 共 1 页	
	文件编号	GL DM-56-18-en			
文件名称： <p style="text-align: center;">CONTROL DM-6D 6D1023 2023-12-10</p> 适用范围：1116 项目					
编制：石哲臣 日期：2023.09.27		审核：刘金盈 日期：2023.09.27		批准：郑剑通 日期：2023.09.27	
修 订 记 录					
版本	TCN/ECR/PCN 编号	修订内容概要	修改人	批准人	批准日期
V3.5.0	/	新建	石哲臣	郑剑通	2023.09.27
发至：	<input type="checkbox"/> 总经办 <input type="checkbox"/> 质量部 <input type="checkbox"/> 财务部 <input checked="" type="checkbox"/> 营销部 <input checked="" type="checkbox"/> 客服 <input type="checkbox"/> 计划 <input type="checkbox"/> 采购 <input checked="" type="checkbox"/> 工程 <input type="checkbox"/> 仓库 <input checked="" type="checkbox"/> 设备研发 <input checked="" type="checkbox"/> 试剂研发 <input type="checkbox"/> 物料质量 <input type="checkbox"/> 设备生产 <input type="checkbox"/> 试剂生产 <input checked="" type="checkbox"/> 试剂质检 <input checked="" type="checkbox"/> 设备质检				
由试剂研发					

DM-6D

HEMATOLOGY CONTROL

Reference Values provided by DYMIND


CONTROL
 2023-09-12

 2023-12-10


Instruments	Parameter	Unit	LOT	6D1023L	LOT	6D1023N	LOT	6D1023H
DYMIND DH-600 DH-602 DH-605 DH-610 DH-612 DH-615 (Technical File Version A2.0 or higher)	WBC	×10 ⁹ /L	4.32	±1.20	7.90	±1.80	22.06	±3.00
	Neu#	×10 ⁹ /L	3.00	±0.40	4.86	±0.80	15.32	±2.00
	Lym#	×10 ⁹ /L	0.64	±0.40	2.14	±0.70	4.62	±1.80
	Mon#	×10 ⁹ /L	0.40	±0.40	0.50	±0.50	0.95	±0.80
	Eos#	×10 ⁹ /L	0.27	±0.40	0.40	±0.70	1.17	±1.60
	Bas#	×10 ⁹ /L	3.48	±0.40	5.71	±0.70	16.28	±1.60
	IG#	×10 ⁹ /L	0.55	±0.50	0.90	±1.00	2.72	±2.50
	Neu%	%	69.5	±12.0	61.5	±12.0	69.4	±12.0
	Lym%	%	14.9	±10.0	27.1	±10.0	20.9	±10.0
	Mon%	%	9.3	±8.0	6.3	±8.0	4.3	±8.0
	Eos%	%	6.3	±10.0	5.1	±10.0	5.3	±10.0
	Bas%	%	80.5	±10.0	72.2	±10.0	73.8	±10.0
	IG%	%	12.8	±10.0	11.4	±10.0	12.4	±10.0
	RBC	×10 ¹² /L	2.39	±0.20	4.57	±0.30	5.36	±0.50
	HGB	g/L	65	±4	136	±6	175	±8
	HCT	%	18.9	±2.0	39.3	±2.5	50.9	±3.0
	MCV	fL	78.9	±5.0	86.1	±5.0	94.9	±5.0
	MCH	pg	27.2	±2.5	29.7	±2.5	32.7	±2.5
	MCHC	g/L	344	±30	345	±30	345	±30
	RDW-CV	%	17.0	±5.0	15.2	±5.0	14.5	±6.0
	RDW-SD	fL	49.6	±10.0	48.5	±10.0	50.6	±12.0
	PLT	×10 ⁹ /L	72	±20	288	±45	583	±65
	MPV	fL	7.2	±3.0	7.2	±3.0	7.2	±3.0
	PDW	fL	8.3	±5.0	8.5	±5.0	8.8	±5.0
	PCT	%	0.052	±0.050	0.206	±0.100	0.421	±0.200
	P-LCR	%	10.5	±20.0	9.6	±20.0	10.0	±20.0
	P-LCC	×10 ⁹ /L	8	±10	27	±30	58	±50
IPF	%	2.0	±2.0	1.5	±1.5	1.7	±1.7	

【NOTE】


1. The controls should be stored in refrigerator (2°C~8°C). After opening, it will keep stable for 14 days when it is stored airtight at 2°C~8°C.
2. Before mixing and running the control after take it out from the refrigerator, please keep it at least 15 minutes until reaching room temperature(15°C~30°C).
3. Controls must be well mixed before using. Please mix gently, to avoid cells rupture and/or generating bubbles.
4. After using, put the controls back into the refrigerator to prevent contamination and evaporation.

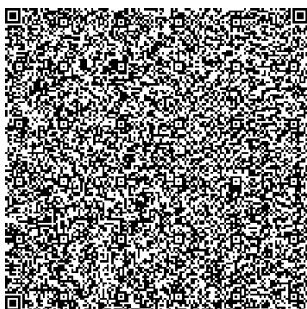

6D1023L

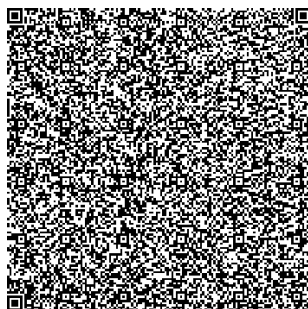

6D1023N

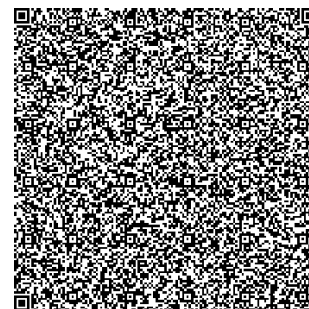

6D1023H