	文件类型	技术文件	文件版本	V3.6.0	
	项目代号	/	页 码	第 0 页 共 1 页	
	文件编号	GL DM-56-18-en			
文件名称： <p style="text-align: center;">CONTROL DM-6D 6D1223 2024-02-10</p> 适用范围：1116 项目					
编制：王雨婷 日期：2023.12.06		审核：刘金盈 日期：2023.12.06		批准：郑剑通 日期：2023.12.06	
修 订 记 录					
版本	TCN/ECR/PCN 编号	修订内容概要	修改人	批准人	批准日期
V3.6.0	/	新建	王雨婷	郑剑通	2023.12.06
发至：	<input type="checkbox"/> 总经办 <input type="checkbox"/> 质量部 <input type="checkbox"/> 财务部 <input checked="" type="checkbox"/> 营销部 <input checked="" type="checkbox"/> 客服 <input type="checkbox"/> 计划 <input type="checkbox"/> 采购 <input checked="" type="checkbox"/> 工程 <input type="checkbox"/> 仓库 <input checked="" type="checkbox"/> 设备研发 <input checked="" type="checkbox"/> 试剂研发 <input type="checkbox"/> 物料质量 <input type="checkbox"/> 设备生产 <input type="checkbox"/> 试剂生产 <input checked="" type="checkbox"/> 试剂质检 <input checked="" type="checkbox"/> 设备质检				
由试剂研发					

DM-6D

HEMATOLOGY CONTROL

Reference Values provided by DYMIND

CONTROL


📅 2023-11-13

🕒 2024-02-10


Instruments	Parameter	Unit	LOT	6D1223L	LOT	6D1223N	LOT	6D1223H
DYMIND DH-600 DH-602 DH-605 DH-610 DH-612 DH-615 (Technical File Version A2.0 or higher)	WBC	×10 ⁹ /L	4.25	±1.20	7.75	±1.80	22.25	±3.00
	Neu#	×10 ⁹ /L	2.97	±0.40	4.92	±0.80	15.74	±2.00
	Lym#	×10 ⁹ /L	0.61	±0.40	1.86	±0.70	4.32	±1.80
	Mon#	×10 ⁹ /L	0.42	±0.40	0.58	±0.50	0.95	±0.80
	Eos#	×10 ⁹ /L	0.25	±0.40	0.40	±0.70	1.24	±1.60
	Bas#	×10 ⁹ /L	3.41	±0.40	5.79	±0.70	16.61	±1.60
	IG#	×10 ⁹ /L	0.58	±0.50	0.98	±1.00	2.90	±2.50
	Neu%	%	69.9	±12.0	63.4	±12.0	70.8	±12.0
	Lym%	%	14.4	±10.0	24.0	±10.0	19.4	±10.0
	Mon%	%	9.9	±8.0	7.5	±8.0	4.3	±8.0
	Eos%	%	5.8	±10.0	5.1	±10.0	5.6	±10.0
	Bas%	%	80.2	±10.0	74.7	±10.0	74.6	±10.0
	IG%	%	13.6	±10.0	12.6	±10.0	13.0	±10.0
	RBC	×10 ¹² /L	2.39	±0.20	4.47	±0.30	5.34	±0.50
	HGB	g/L	63	±4	133	±6	174	±8
	HCT	%	18.4	±2.0	39.8	±2.5	51.8	±3.0
	MCV	fL	76.9	±5.0	89.0	±5.0	96.9	±5.0
	MCH	pg	26.1	±2.5	29.9	±2.5	32.5	±2.5
	MCHC	g/L	340	±30	336	±30	335	±30
	RDW-CV	%	16.1	±5.0	14.5	±5.0	14.1	±6.0
	RDW-SD	fL	45.7	±10.0	47.6	±10.0	50.6	±12.0
	PLT	×10 ⁹ /L	72	±20	295	±45	552	±65
	MPV	fL	7.3	±3.0	7.3	±3.0	7.3	±3.0
	PDW	fL	8.6	±5.0	8.9	±5.0	9.5	±5.0
	PCT	%	0.052	±0.050	0.214	±0.100	0.403	±0.200
	P-LCR	%	11.4	±20.0	10.8	±20.0	10.5	±20.0
	P-LCC	×10 ⁹ /L	8	±10	32	±30	58	±50
IPF	%	2.5	±2.5	2.1	±2.1	1.7	±1.7	

【NOTE】


1. The controls should be stored in refrigerator (2°C~8°C). After opening, it will keep stable for 14 days when it is stored airtight at 2°C~8°C.
2. Before mixing and running the control after take it out from the refrigerator, please keep it at least 15 minutes until reaching room temperature(15°C~30°C).
3. Controls must be well mixed before using. Please mix gently, to avoid cells rupture and/or generating bubbles.
4. After using, put the controls back into the refrigerator to prevent contamination and evaporation.

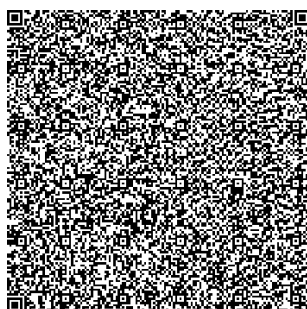

6D1223L

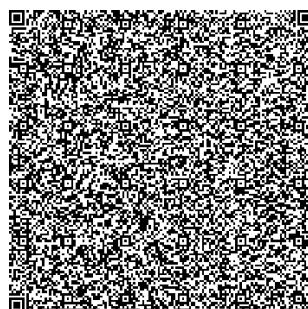

6D1223N

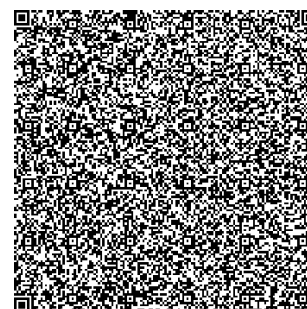

6D1223H